

# **Medical Image Reconstruction**

## **Term II - 2012**

### **Topic 4:**



## **Motion Artifacts**

Professor Yasser Mostafa Kadah

# MRI Data Acquisition

---


- ▶ MR image is acquired in the k-space
- ▶ Reconstruction is an inverse Fourier transformation
- ▶ Parts of k-space are acquired at different times

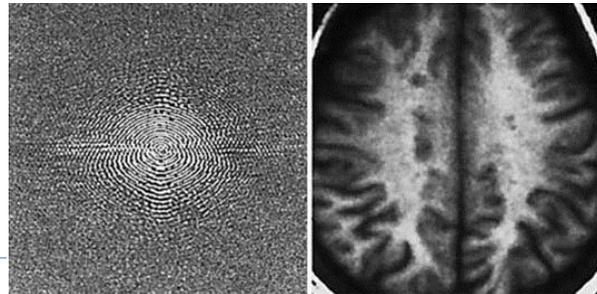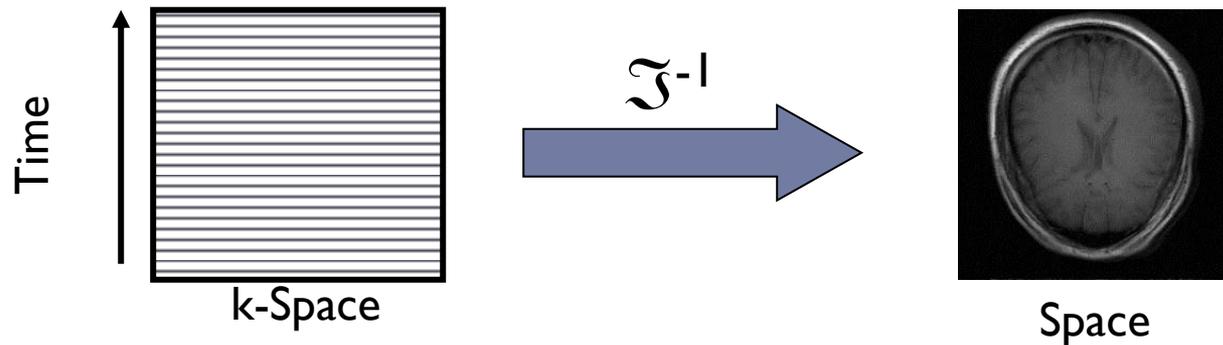

# Motion Artifact in MRI

---

- ▶ Motion artifacts result when the patient moves during MR acquisition
  - ▶ **Physiological/voluntary motion**
- ▶ Motion artifact manifests itself in the image as severe blurring that usually mandates the scan to be repeated
  - ▶ **Costly in addition to added discomfort to the patient**
- ▶ Postprocessing techniques can be used
  - ▶ **Time consuming and inefficient in many cases**
  - ▶ **No considered practical for clinical use**

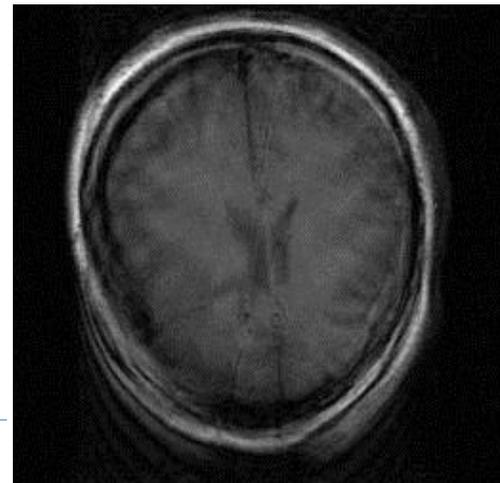

# Types of Motion Artifacts


---

- ▶ Intra-slice: motion during acquisition of a slice
  - ▶ causes k-space of a given image to contain magnitude and phase errors
- ▶ Inter-slice: motion in between acquisition of whole slices
  - ▶ causes repeated acquisitions of the same slice to be different
- ▶ These two types have been treated separately in the literature
- ▶ Inter-slice motion is simpler to correct for using registration techniques (e.g., AIR)




Average

Inter-Slice

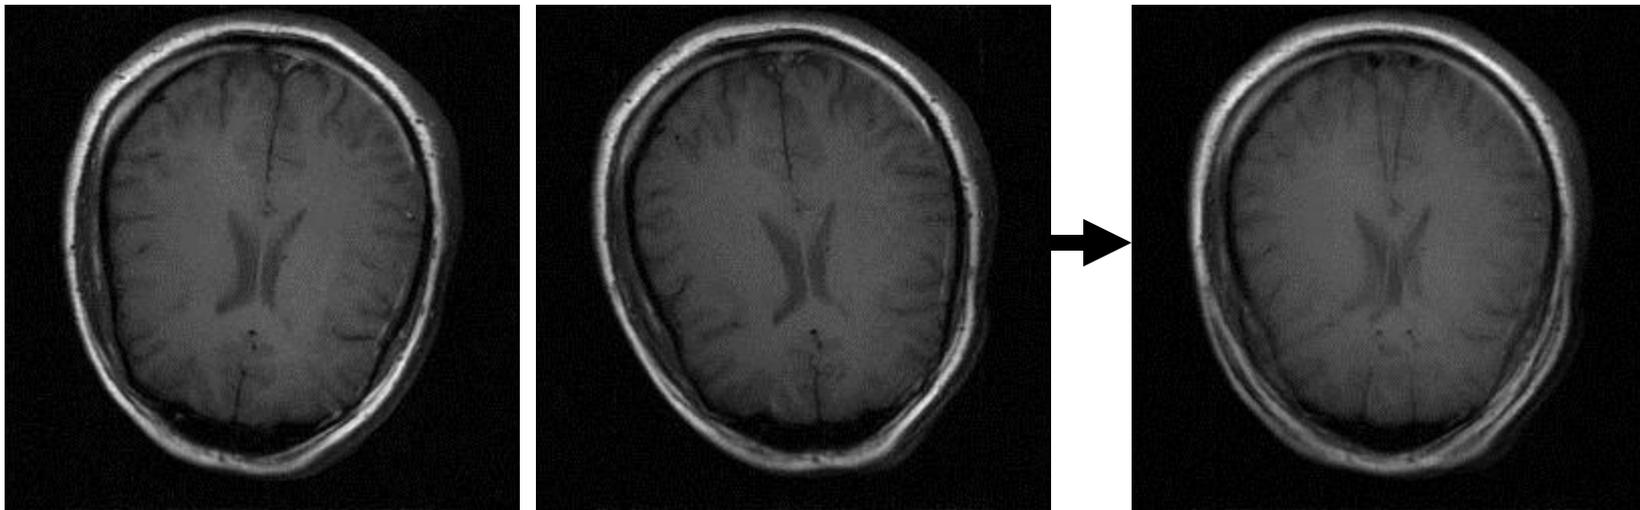

Intra-Slice

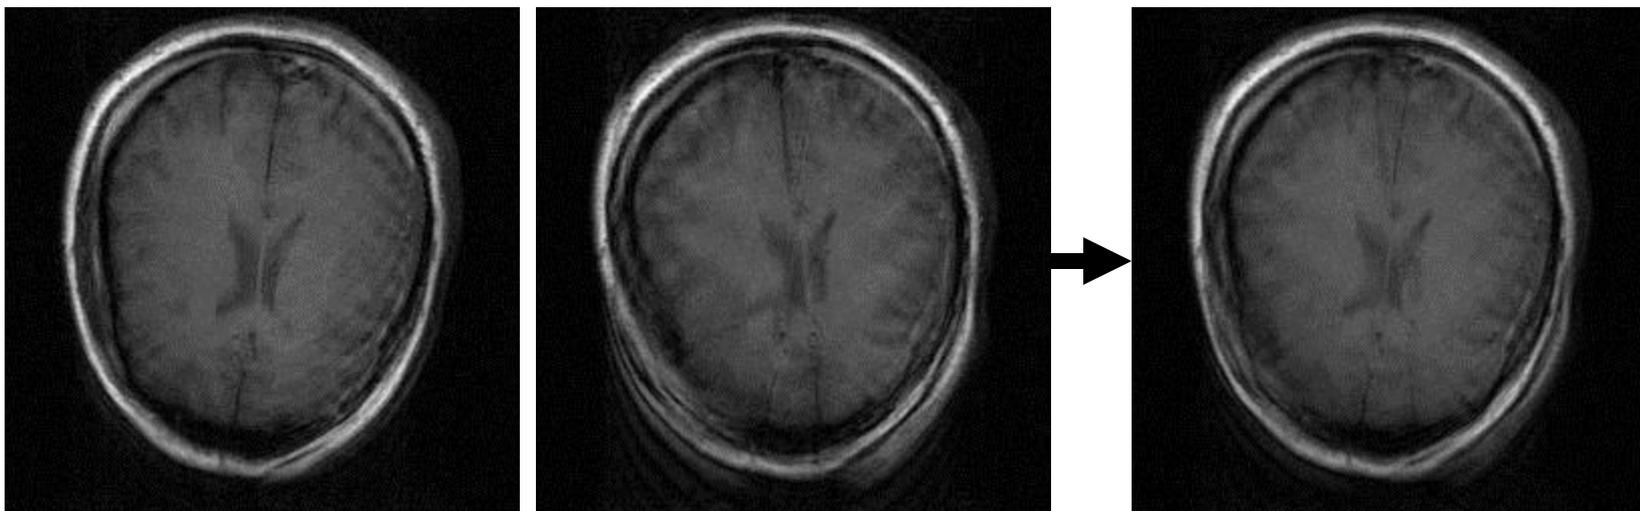

# Intra-Slice Motion Suppression


---

- ▶ Intra-slice motion artifact suppression is a challenging problem
  - ▶ k-space “pieces” are more difficult to register!
- ▶ Among the most successful techniques used to estimate motion is the navigator echo (NAV) technique.
  - ▶ Most practical for clinical use.
- ▶ The original formulation relies on acquiring an extra line in the center of k-space along the  $k_x$  or  $k_y$  directions to detect motion in that direction.



# Classical Navigator Echo\*

- ▶ Acquire the navigator (NAV) echo line in the center of the k-space with every k-space section.
  - ▶ Each represents the Fourier transform of a projection of the image
- ▶ Register the two NAV lines together to estimate motion along the NAV direction

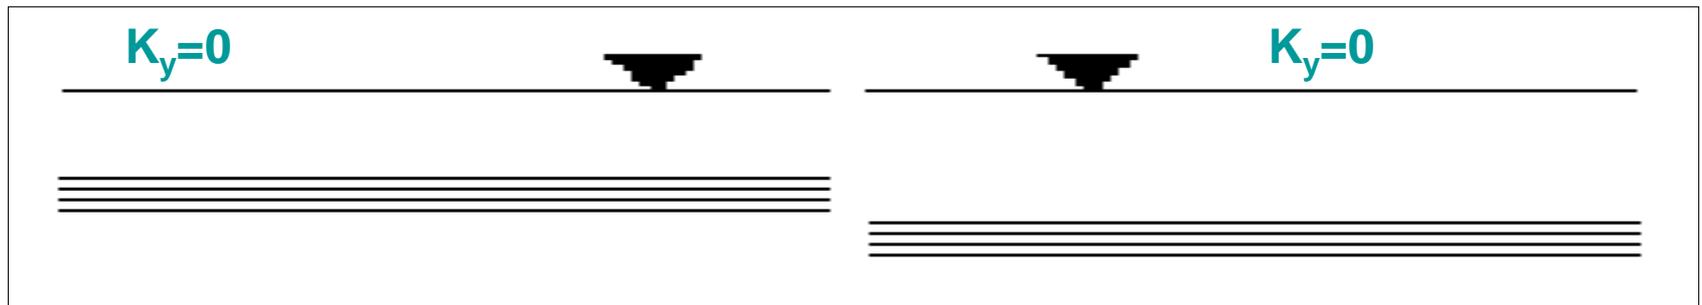

\* Felmlee and Ehman, *Magn. Reson. Med.*, 1992

# Limitations of NAV


---

- ▶ Requires an extra amount of time to acquire this line prior to actual k-space acquisition
  - ▶ limits the minimum TE of such sequences
  - ▶ Additional complexity in sequence programming
- ▶ The estimation of motion parameters in both the read-out and phase encoding directions is not possible with a single line.
  - ▶ Two NAV lines in orthogonal directions must be used
  - ▶ Circular and spherical NAV for 2- and 3-D estimation



# Floating Navigator Echo (fNAV)\*


- ▶ Instead of acquiring the navigator echo line in the center of the k-space, we acquire this line by acquiring k-space sections that overlap in a single line.
- ▶ Enables the estimation of 2-D translational motion
- ▶ Rotation cannot be estimated

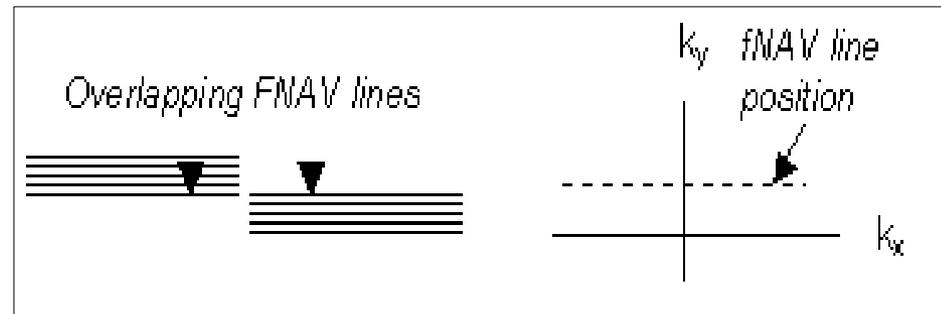

\* Kadah et al, *Magn. Reson. Med.*, 2004

# Arc Navigator Echo (aNAV)\*

- ▶ A fast way to compute the rotational motion is to match points on an arc within the area of overlap rather than the whole area.
- ▶ Similar in theory to orbital navigator echo (ONAV)

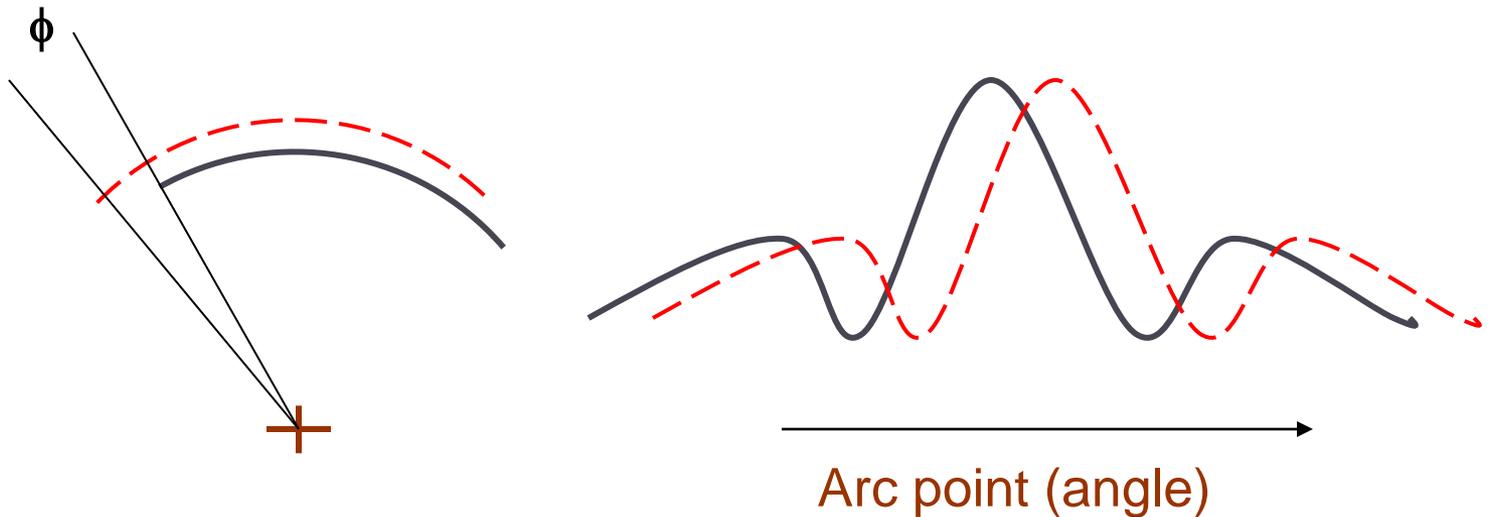

\* Mohamed, Youssef and Kadah, *Proc. SPIE Med. Imag. 2003*

# Reconstruction Method


## Overlapped k-Space Acquisition and Reconstruction Technique for Motion Artifact Reduction in Magnetic Resonance Imaging

Yasser M. Kadah


- ▶ Address the problems of intra-slice and inter-slice motion together
  - ▶ For example, when segmented acquisition is used with  $NEX > 1$
- ▶ To propose an extension of the fNAV to allow rotation to be estimated
  - ▶ Acquisition of navigator “area” rather than “line” or “arc”
  - ▶ Take advantage of the extra data acquisition when  $NEX$  is required to be  $> 1$  to estimate the intra-slice motion
  - ▶ Maintain efficiency by not acquiring extra data other than those required for averaging

# Basic Idea

## Conventional Acquisition Method

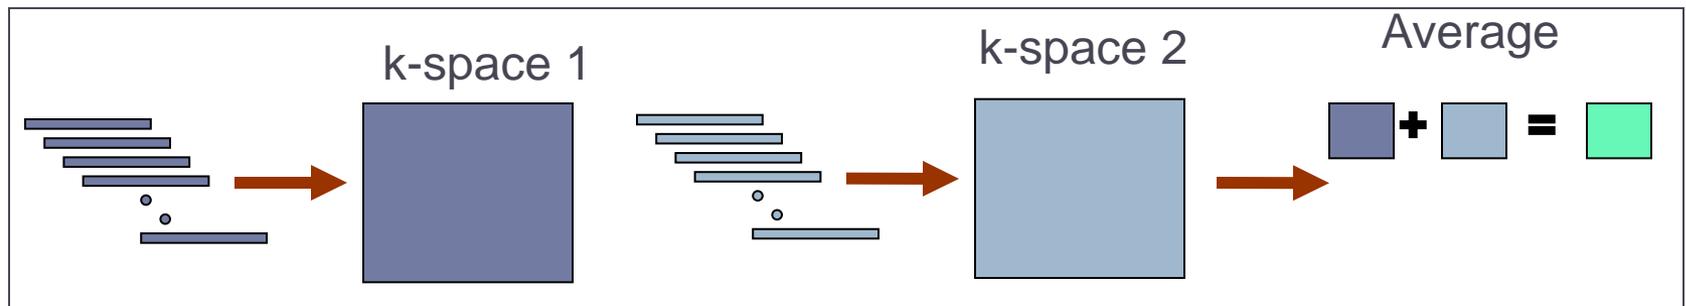


## New Acquisition Method

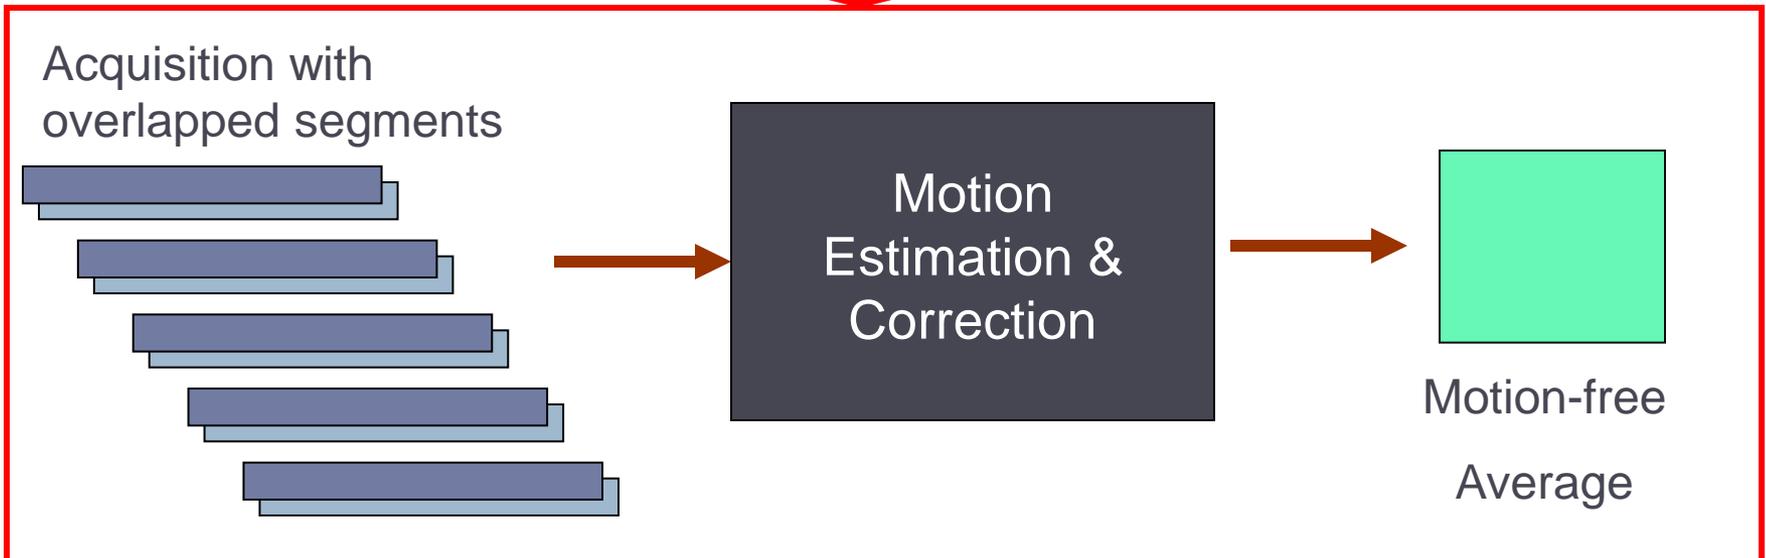

# Motion Estimation


---

- ▶ Identify the area of overlap under the assumption of a general in-plane rigid body transformation
- ▶ Estimate rotation from magnitude of overlap area
  - ▶ Correlation based methodology
- ▶ Estimate translation from phase of overlap area
  - ▶ fNAV estimation method

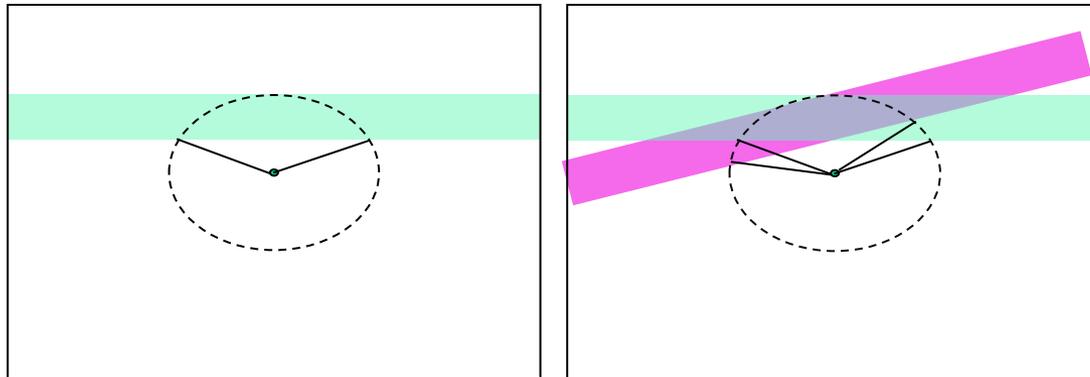

# Proposed Method

---

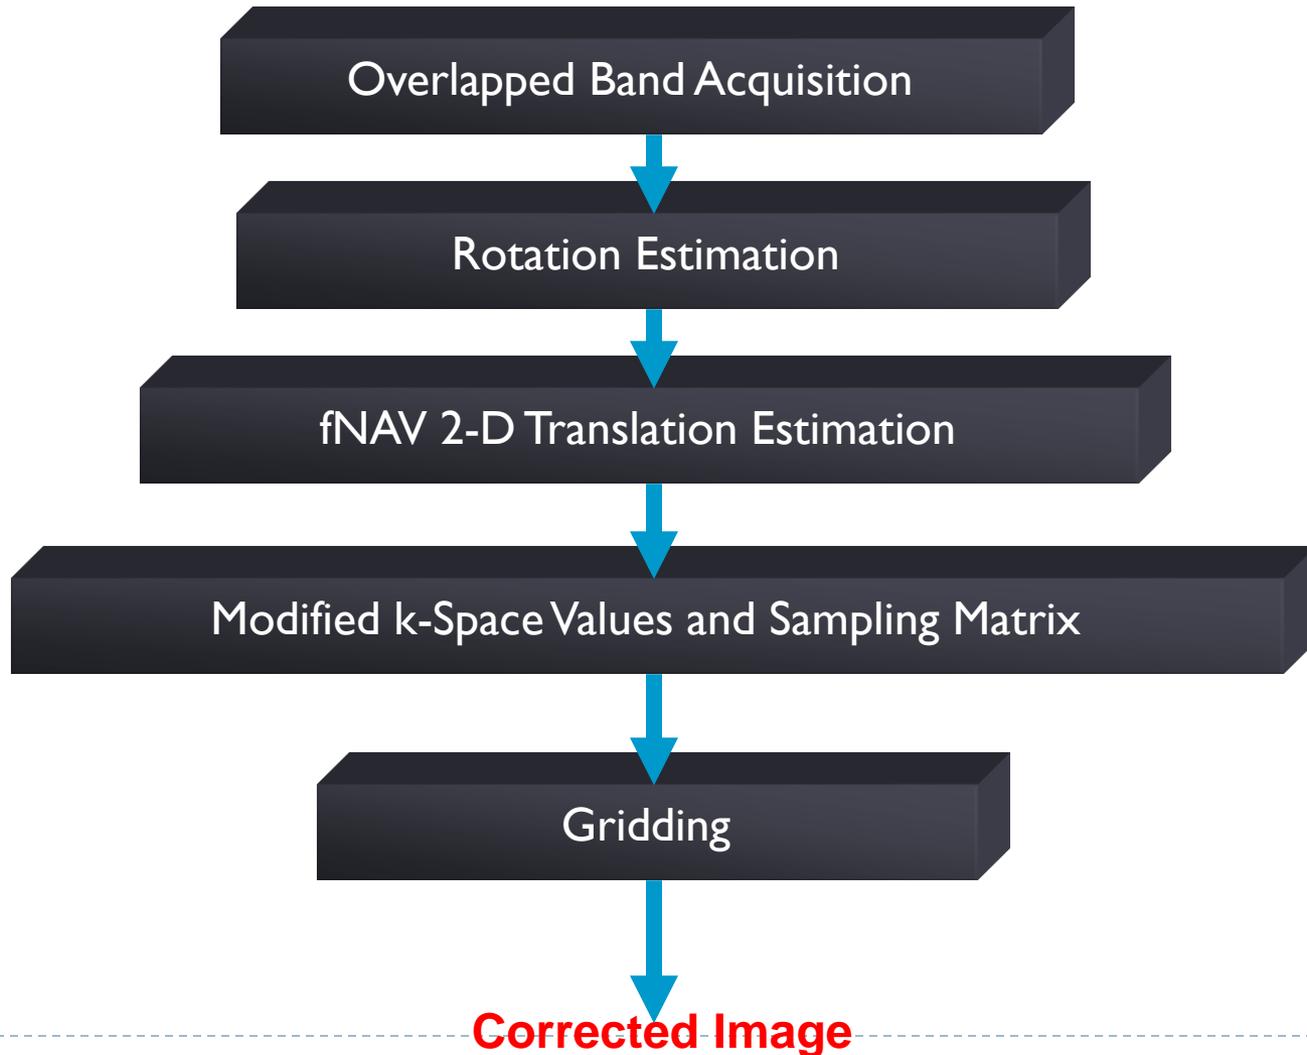

# Experimental Verification Using Numerical Simulations

---


- ▶ Simulated motion data were obtained from evaluating the analytical form of the Shepp-Logan phantom with different motion as well as simulating motion on real MRI head images.
  - ▶ Matrix: 128, Band size=16 with 50% overlap.
  - ▶ Random translational and rotational motion parameters were simulated for each band
- ▶ Reconstruction is performed using conventional gridding method to account for nonuniformity of sampling after motion




# Simulated Data

## ▶ Estimated vs. real motion


Translation

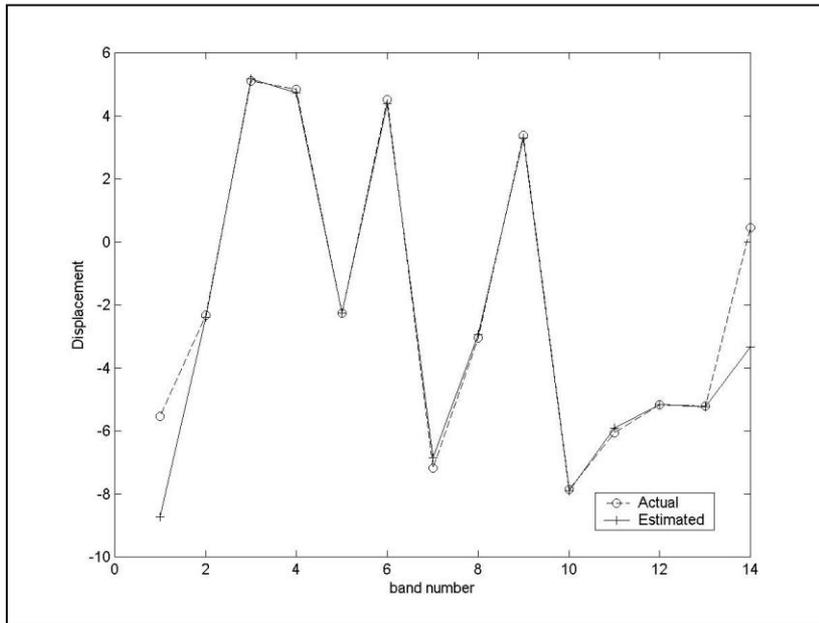


Rotation

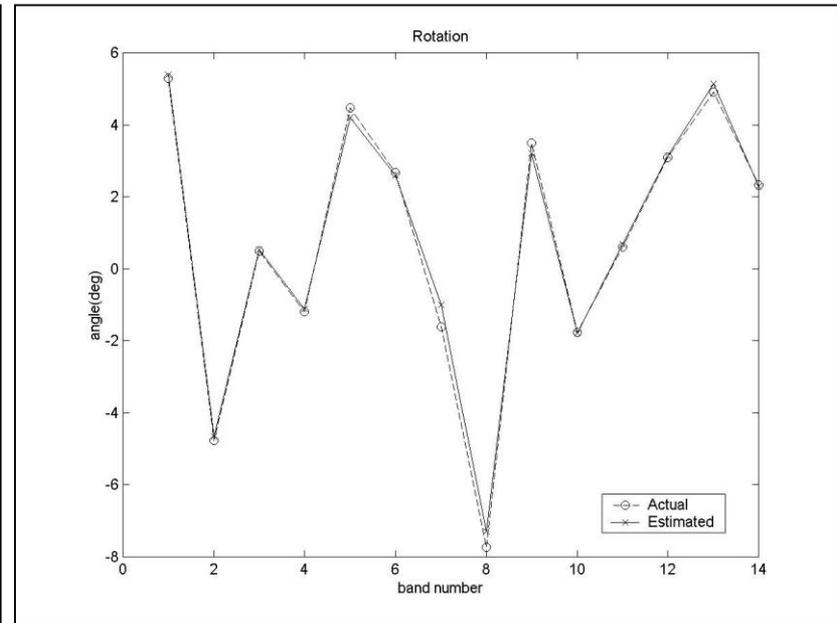


Distorted

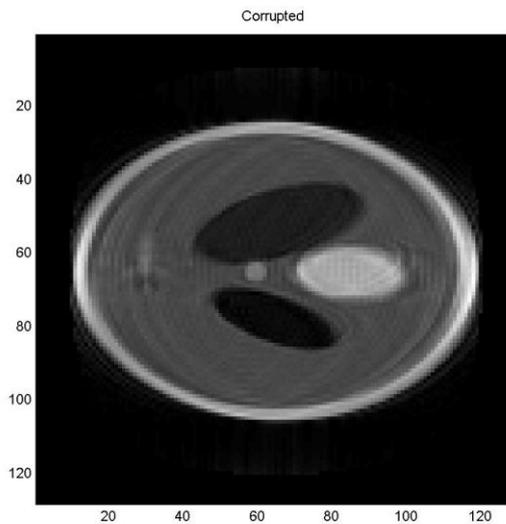


Corrected

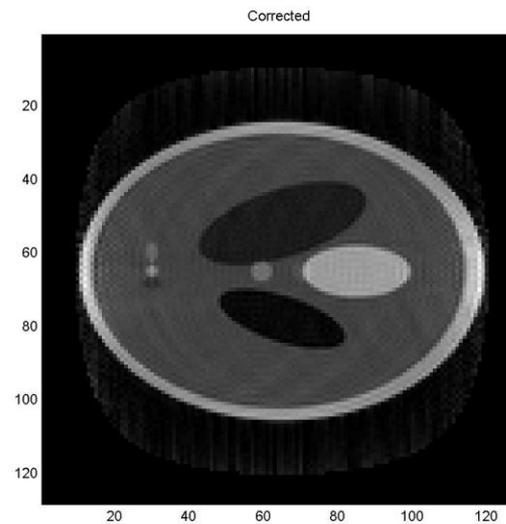


Distorted

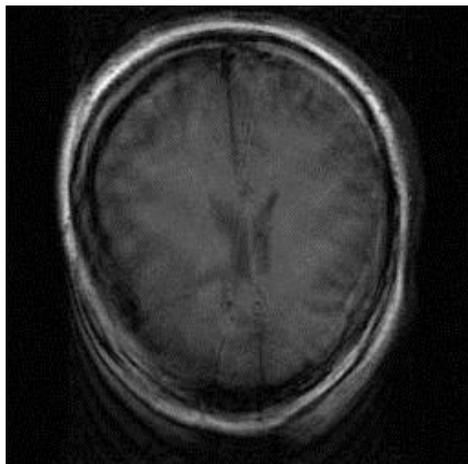

Corrected

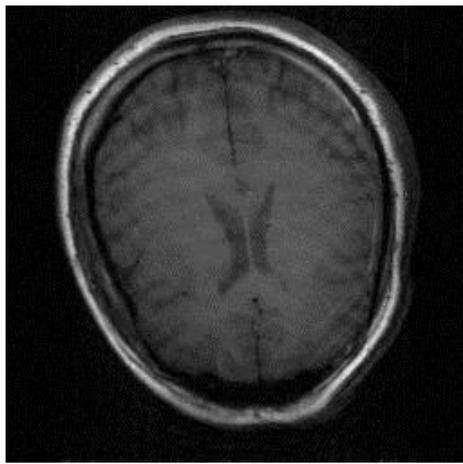

Motion-free

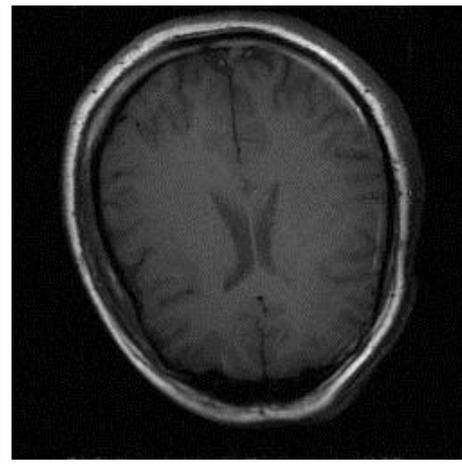

# Experimental Verification Using Real MRI Data

---

- ▶ Real data were obtained from a Siemens Magnetom Trio 3.0T MR system\*
  - ▶ Matrix  $256 \times 224$
  - ▶ ETL=16, NEX=2
  - ▶ Overlap of 50% was used
  - ▶ Normal human volunteer instructed to move once in the middle of acquisition
- ▶ Reconstruction is performed using conventional gridding method to account for nonuniformity of sampling after motion


---

▶ \* Acquired by author at BITC - Emory/Georgia Tech Biomedical Engineering, Atlanta, GA, U.S.A.

# Real Data

---

No Motion

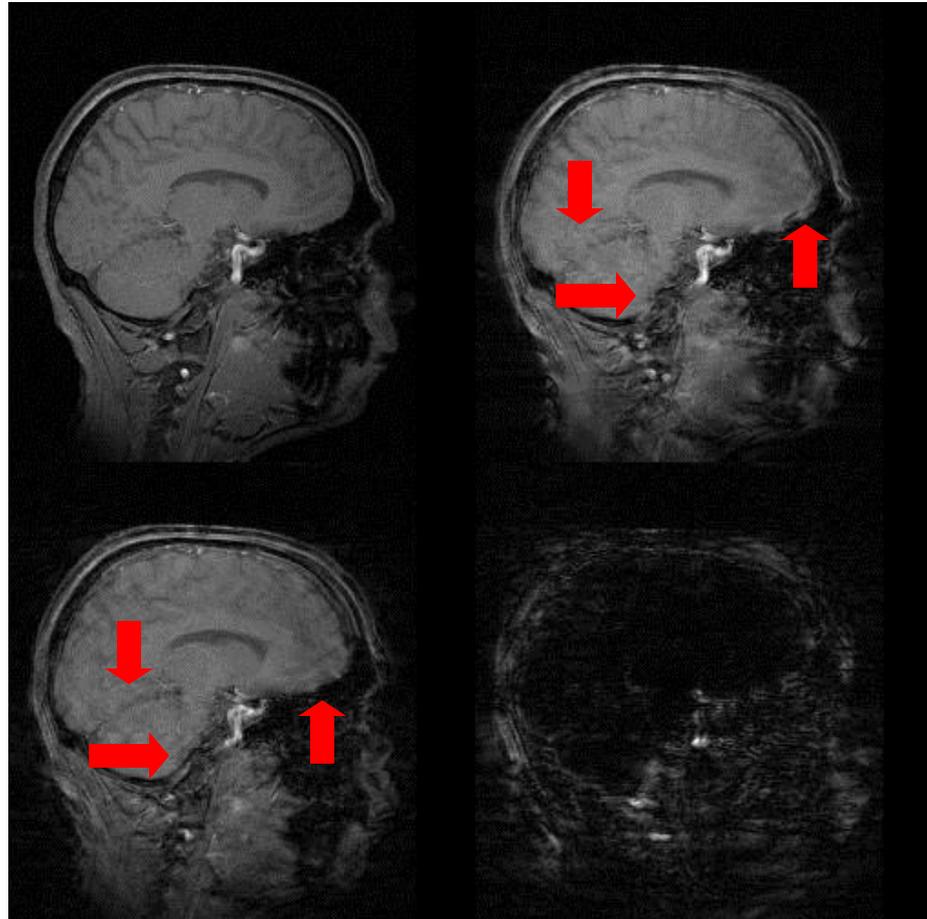

Motion  
Distorted

Corrected


Difference  
between  
Corrected and  
Distorted



# Discussion

---

- ▶ Two problems were observed in the reconstruction phase of the developed method
- ▶ Problem 1: Existence of k-space voids
  - ▶ Missing k-space data
  - ▶ Undesired variations in the SNR within k-space
- ▶ Problem 2: Long reconstruction time
  - ▶ Rotation requires regridding according to estimated motion
  - ▶ A new reconstruction table has to be computed each time

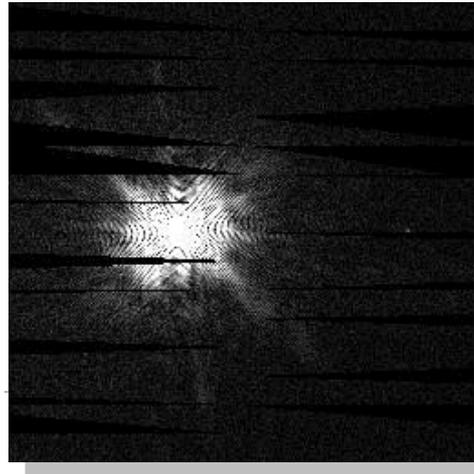

# Exercise

---

- ▶ Write a short literature review section on the methods used for inter-slice motion correction in MRI with references.
- ▶ Would the proposed method be possible to extend for use with CT data where acquisition lines are radial? Explain your answer.
- ▶ Use the data set on the class web site to show that 2D translational motion does not affect the magnitude of k-space and that such motion can be estimated by correlation based method.
- ▶ Do a literature search on the topic of motion artifacts in ONE medical imaging modality of your choice and come up with a list of relevant references related to the subject including both research papers and patents.

